


PRO-SERIES RESET PROCEDURE



ELITEpro RESET and GND Pins

1. Remove voltage leads from any source!
2. Do not remove original battery if the unit has valuable data stored!
3. Remove the four case screws from the bottom panel
4. Slide the top panel off the end panels and lay to the side
5. Short RESET and GND pins for one second
6. Both LEDs should flash briefly, and then go dark. If LEDs continue to flash repeatedly, please contact DENT Instruments as your logger may require further repair.
7. Close the case and re-install the four case screws
8. Connect with ELOG software

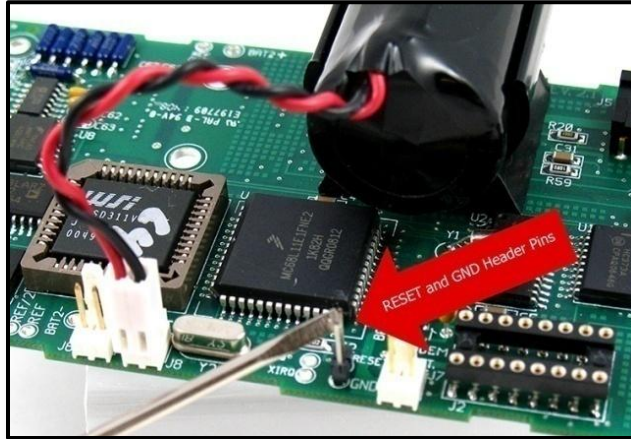

DATApr RESET and GND Pins

